

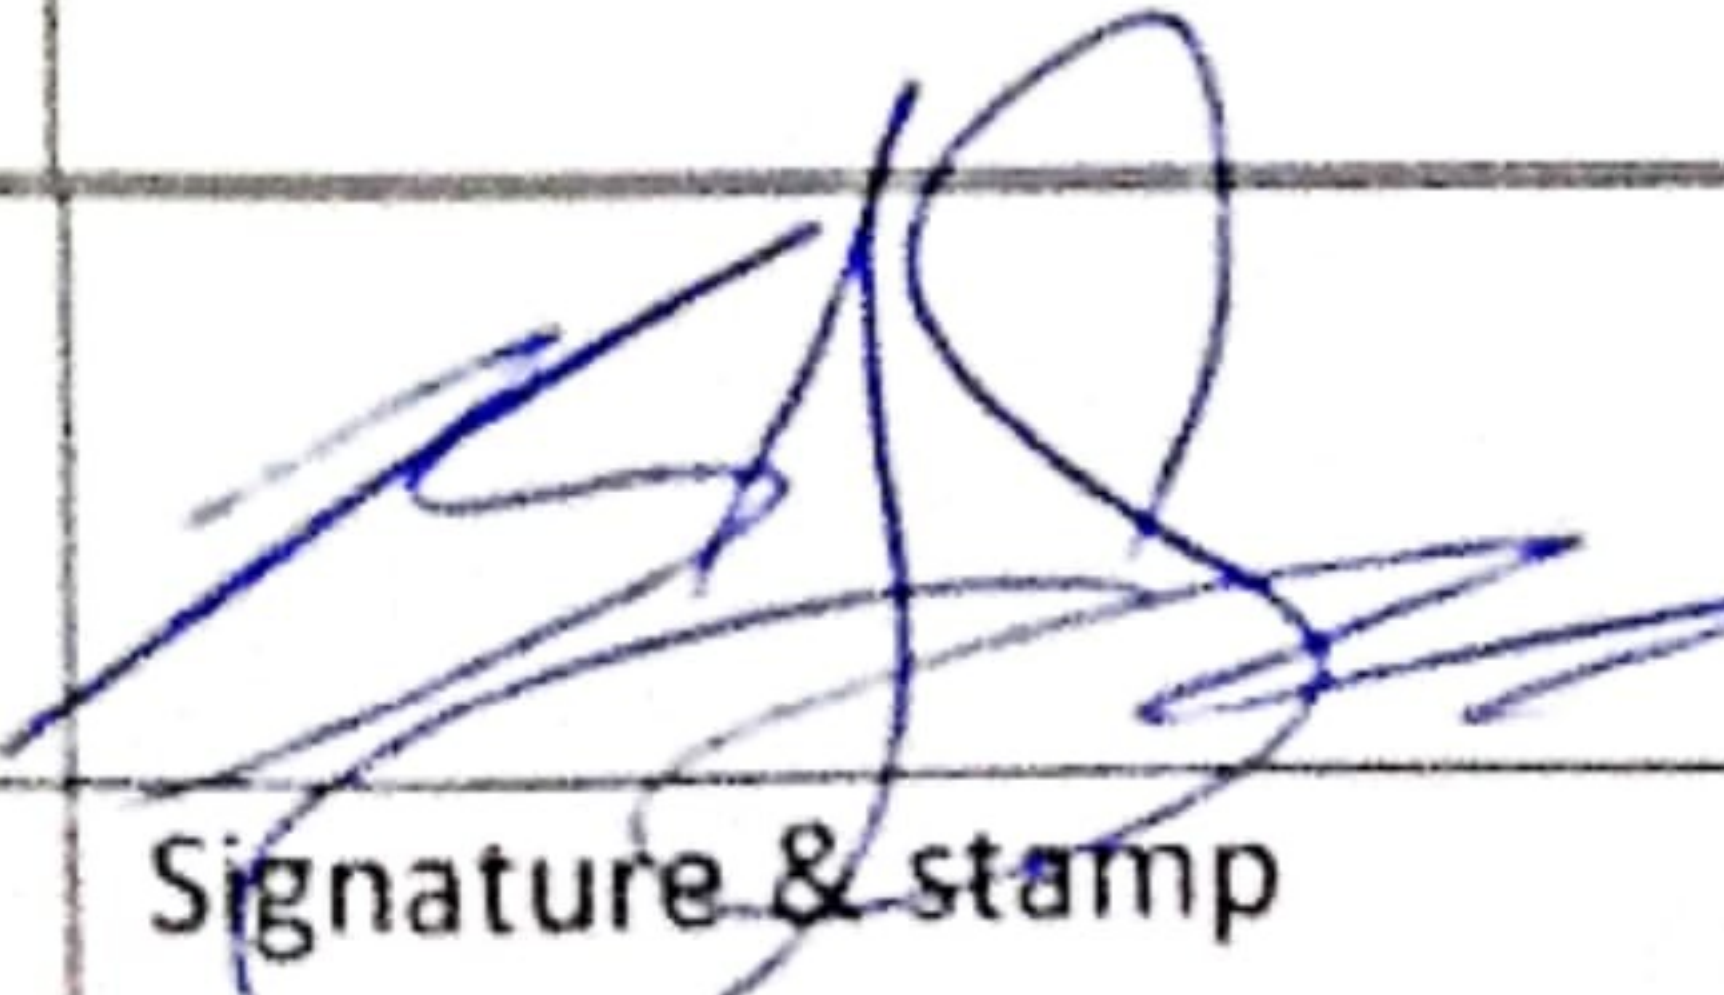



Cygnus Instruments, Inc.
6900 Philips Highway
Suite 8
Jacksonville FL 32216

Tel: 410-267-9771

E-mail: Sales@Cygnusinstruments.com
Web: www.CygnusInstruments.com

Certificate of Test & Calibration

Calibration Date	November 03, 2021																
Calibration Due Date	November 03, 2023																
Calibration Report Number/Certificate Number	8821																
Customer	KROLMARK MARINE SERVICES, S.A. 5676 CALLE C. SUR EL CARMEN DAVID 0426-00517 CHIRIQUI PANAMA																
Equipment	Hatch Sure Leak Inspection Receiver, Transmitter, and Microphones																
Receiver Serial Number	RX1256																
Transmitter Serial Number	TX1256																
Details	<p>Receiver tested for functionality and calibrated against a dB signal source.</p> <table border="1"> <thead> <tr> <th>Source dB</th> <th>Meas. dB</th> <th>Accepted limits</th> </tr> </thead> <tbody> <tr> <td>0dB</td> <td>0</td> <td>+/- 1dB</td> </tr> <tr> <td>20dB</td> <td>20</td> <td>+/- 1dB</td> </tr> <tr> <td>40dB</td> <td>40</td> <td>+/- 1dB</td> </tr> <tr> <td>60dB</td> <td>60</td> <td>+/- 1dB</td> </tr> </tbody> </table> <p>Transmitter elements tested OH calibration tested All other items tested</p>		Source dB	Meas. dB	Accepted limits	0dB	0	+/- 1dB	20dB	20	+/- 1dB	40dB	40	+/- 1dB	60dB	60	+/- 1dB
Source dB	Meas. dB	Accepted limits															
0dB	0	+/- 1dB															
20dB	20	+/- 1dB															
40dB	40	+/- 1dB															
60dB	60	+/- 1dB															
Calibration Equipment Used	TG2000 Serial No. 342715 – Calibrated – certificate #1062119 PL310 Serial No. 034651 – Calibrated – certificate #2062119 PicoScope 3204 Serial No. YSR75/095																
Bryan Sanders	 																
Calibrated by	Signature & stamp	Date															
		11/03/21															